CIOD I CR, IIIC.	Drawing Title: Nema 5-15P hospital grade with green dot to IEC60320 C13 2 CONDUCTORS + GROUND, GT Cable #104: 14 / 3 Conductors, 9.3mm OD, SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL, 3700 +/- 50mm, GlobTek Black	
•	Model No. Power Cord	
Northvale, NJ 07647		
Tel. (201) 784-1000	Part No./Ordering No. 11910412F701-1	Rev D2
Fax (201) 784-0111		

In Addition to GlobTek Inc.'s renewed ISO9001:2008 - Quality Management System Certification, GlobTek Inc. is now certified to:

ISO13485:2003 - Medical Devices Quality Management System Certification

ISO14001:2004 - Environmental Management System Certification

ISO Certificates are available online at https://www.globtek.com/iso-certificates/

Prop 65 Statement:https://en.globtek.com/prop-65-statement.pdf

The acceptance of this specification and use of the product described in this document indicates the acceptance and binding of the customer to Globtek TERMS AND CONDITIONS (attached to the end of this document), which supersede all other agreements, terms, and conditions (<a href="https://en.globtek.com/terms-and-conditions/">https://en.globtek.com/terms-and-conditions/</a>).

The purchaser of this product (Customer) agrees that it is their sole responsibility to determine suitability/fitness of the product described in this specification for their application and to take precautions for protection against any hazards attendant to the handling and use of the product.

#### Footnote:

GlobTek Inc. will not be liable for the safety and performance of these power supplies if unauthorized access and repair occurs. End user should consult applicable UL, CSA or EN standards for proper installation instruction.

### Limitation of Use:

GlobTek products are intended for use with commercial, medical, and/or industrial equipment only. GlobTek product are not authorized for use as mission critical components in life support hazardous environment, nuclear or aircraft applications without prior written approval from the CEO of GlobTek Inc.

Contents of this document are subject to change without prior notice.

## **Customer Approval of Specification:**

Please approve, sign and send back to GlobTek so we can complete order processing.

A delay in receipt of this form will delay delivery schedule.

Company Name:	Customer P/N:
Quote Number:	Date:
Authorized Representative Name:	Authorized Representative Signature:

CIOD I CR, IIIC.	Drawing Title: Nema 5-15P hospital grade with green dot to IEC60320 C13 2 CONDUCTORS + GROUND, GT Cable #104: 14 / 3 Conductors, 9.3mm OD, SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL, 3700 +/- 50mm, GlobTek Black	
•	Model No. Power Cord	
Northvale, NJ 07647		
Tel. (201) 784-1000	Part No./Ordering No. 11910412F701-1	Rev D2
Fax (201) 784-0111		

### **REVISION HISTORY**

REV	DESCRIPTION	SUB	DATE	APPROVED
D2	Correct cable length to 3700±50 mm, update coil dimensions to 280*250 mm	QA	01/05/2021	QA
D1	Correct rating from 12A / 125V~ to 15A / 125V~; Update drawings.	bsiep	11/13/2020	QA
D	Update to SF format; remove customer P/N labels.	bsiep	11/04/2020	QA

Cordset Information:


CordsetColor:GlobTek Black Cord Length (mm):3700 +/- 50

3D File Download https://www.globtek.com/file/dl/11910412F701-1.zip


# NOTES:

Includes "GROUNDING RELIABILITY LABEL" shown in drawing.

CIOD I CIN, IIIO.	Drawing Title: Nema 5-15P hospital grade with green dot to IEC60320 C13 2 CONDUCTORS + GROUND, GT Cable #104: 14 / 3 Conductors, 9.3mm OD, SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL, 3700 +/- 50mm, GlobTek Black	
•	Model No. Power Cord	
Northvale, NJ 07647		
Tel. (201) 784-1000	Part No./Ordering No. 11910412F701-1	Rev D2
Fax (201) 784-0111		

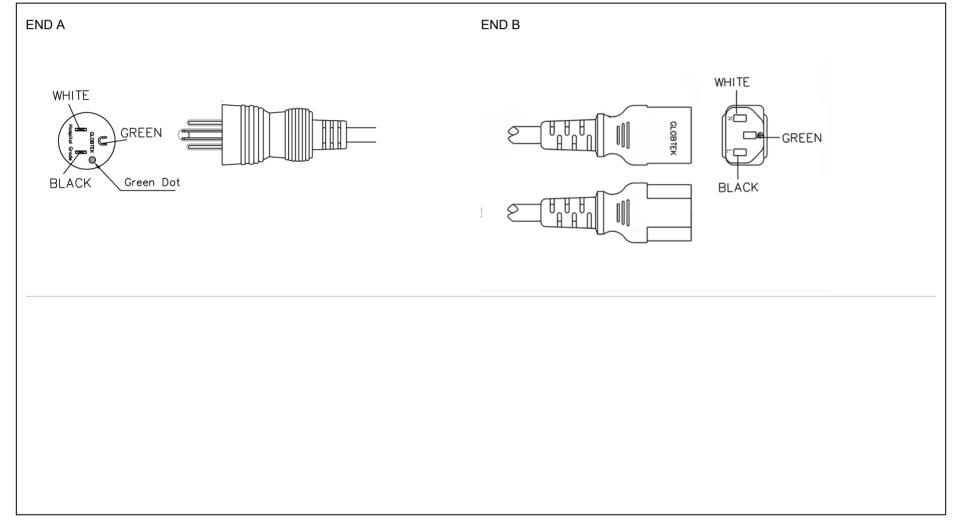

CIOD I CIX, IIIO.	Drawing Title: Nema 5-15P hospital grade with green dot to IEC60320 C13 2 CONDUCTORS + GROUND, GT Cable #104: 14 / 3 Conductors, 9.3mm OD, SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL, 3700 +/- 50mm, GlobTek Black	
•	Model No. Power Cord	
Northvale, NJ 07647		
Tel. (201) 784-1000	Part No./Ordering No. 11910412F701-1	Rev D2
Fax (201) 784-0111		

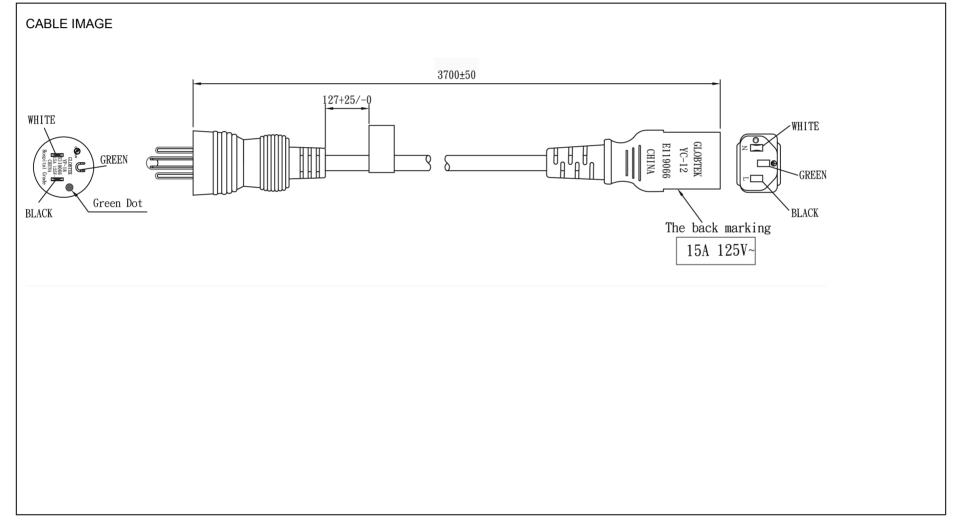

CIOD I CIX, IIIC.	Drawing Title: Nema 5-15P hospital grade with green dot to IEC60320 C13 2 CONDUCTORS + GROUND, GT Cable #104: 14 / 3 Conductors, 9.3mm OD, SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL, 3700 +/- 50mm, GlobTek Black			
	Model No. Power Cord			
Northvale, NJ 07647				
Tel. (201) 784-1000	Part No./Ordering No. 11910412F701-1	Rev D2		
Fax (201) 784-0111				

End A	Cable	End B
Code:119	Code:104	Code:701-125V/15A max
Description:Nema 5-15P hospital grade with green dot	Description:GT Cable #104: 14 / 3 Conductors, 9.3mm OD,	Description:IEC60320 C13 2 CONDUCTORS + GROUND
Rating (V):125	SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL	Rating (V):125
Rating (A):15.0	Color:GlobTek Black	Rating (A):15.0
Gender:Male	Wire Gauge(AWG):14	Gender:Female
Overmolded:Yes	Cond:3	Overmolded:Yes
	Type:SJT	
	Temperature:105° C	
	Amps:15	
	Volts:300	
	OD:9.3	
	ConductorsColors:BLK/WHT/GRN	

Overall cable	rating:15A 125V~
---------------	------------------


Plug Approvals		Cable Approvals		Connector Approvals		
CULUS	UL/CUL	CULUS	UL/CUL	CULUS	UL/CUL	
UL 817 LINK TO CERT		UL 817 LINK TO CERT		UL 817 LINK TO CERT		
AGENCY ONLINE DOCUMENTS	http://ei	n.globtek.com/cordsets/				
RoHS/RoHS3 Declaration	https://\	www.globtek.com/pdf/rohs_cert/01	t30000002p57ZAAQ			
REACH Declaration	https://\	https://www.globtek.com/pdf/iso_certificates/REACH.pdf				
Conflict Minerals Declaration	https://\	https://www.globtek.com/pdf/conflict-minerals.pdf				
Prop 65 Statement	https://e	https://en.globtek.com/prop-65-statement.pdf				
CE.UKCA.Cord	https://ç	https://globtek.secure.force.com/spec/ec_decl_product_model_family_incl_cord?id=01t30000002p57Z				

### PROPRIETARY INFORMATION

CIOD I CIX, IIIO.	Drawing Title: Nema 5-15P hospital grade with green dot to IEC60320 C13 2 CONDUCTORS + GROUND, GT Cable #104: 14 / 3 Conductors, 9.3mm OD, SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL, 3700 +/- 50mm, GlobTek Black	
	Model No. Power Cord	
Northvale, NJ 07647		
Tel. (201) 784-1000	Part No./Ordering No. 11910412F701-1	Rev D2
Fax (201) 784-0111		


IPAY fating is based on 3rd party testing and customers should check suitability and test system level IPAY fating before ordering.

CIOD I CIX, IIIO.	Drawing Title: Nema 5-15P hospital grade with green dot to IEC60320 C13 2 CONDUCTORS + GROUND, GT Cable #104: 14 / 3 Conductors, 9.3mm OD, SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL, 3700 +/- 50mm, GlobTek Black	
	Model No. Power Cord	
Northvale, NJ 07647		
Tel. (201) 784-1000	Part No./Ordering No. 11910412F701-1	Rev D2
Fax (201) 784-0111		

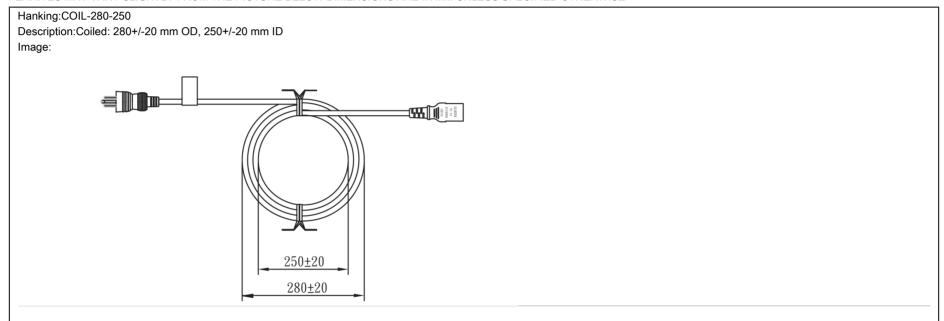

Notes/Modifications/Customizations (notes in this section supersede the values shown in the standard spec):

CIOD I CIX, II IC.	Drawing Title: Nema 5-15P hospital grade with green dot to IEC60320 C13 2 CONDUCTORS + GROUND, GT Cable #104: 14 / 3 Conductors, 9.3mm OD, SJT, 105 Deg.C, 300V, BLK/WHT/GRN, Approvals: UL/CUL, 3700 +/- 50mm, GlobTek Black  Model No. Power Cord		
•			
Northvale, NJ 07647			
Tel. (201) 784-1000	Part No./Ordering No. 11910412F701-1	Rev D2	
Fax (201) 784-0111			

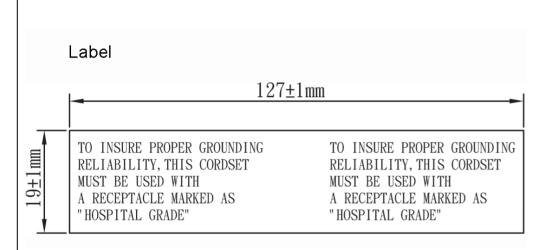

### NOTES:

- 1) PERMANENTLY ATTACHED FLAG LABEL
- 2) BASE MATERIAL: WHITE POLYVINYL CHLORIDE, 0.05mm THICK WITH PERMANENT PRESSURE SENSITIVE ADHESIVE ON ONE SIDE.
- 3) PRINTING: TEXT IS PRINTED IN PERMANENT BLACK INK, LETT HEIGHT IS 2.6mm MINIMUM.